


吉力科技
杭州高压电气技术有限公司
Hangzhou High Voltage Technology Co., Ltd.

WWW.HVTW.COM

135 136 137

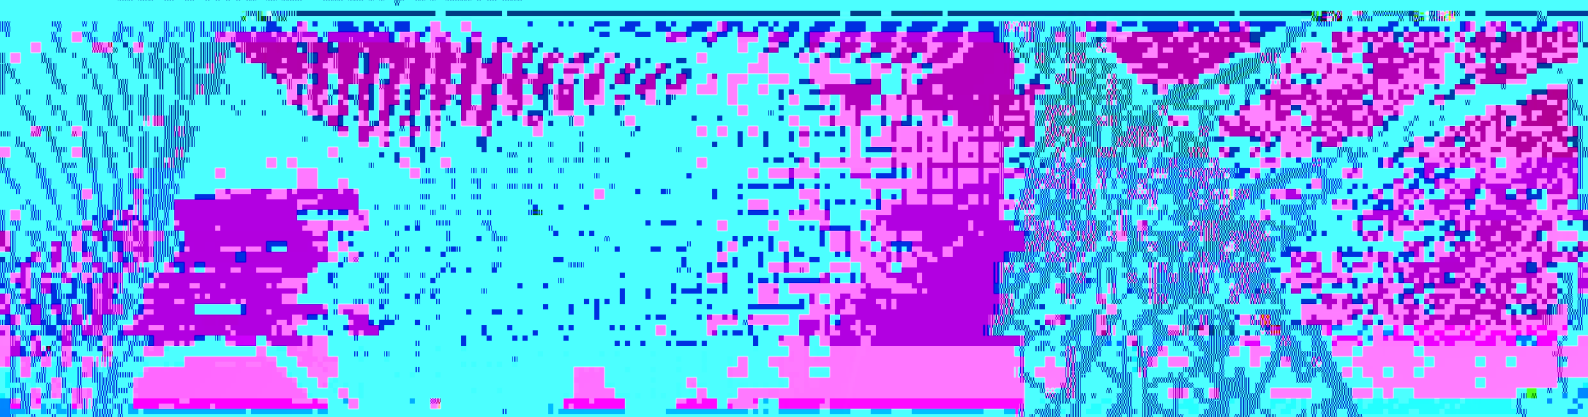

杭州高压电气技术有限公司

C13901

杭州高压电气技术有限公司
Hangzhou High Voltage Technology Co., Ltd.

使用说明书

杭州高压电气技术有限公司

HANGZHOU HIGH VOLTAGE TECHNOLOGY CO., LTD.

电话：0571-89935600 传真：0571-89935608

“ ” 1

168

19

.....	1
.....	2
.....	3
.....	4
.....	8
.....	10
.....	10

1

2

“

”

“


”

1)

2)

3)

4)

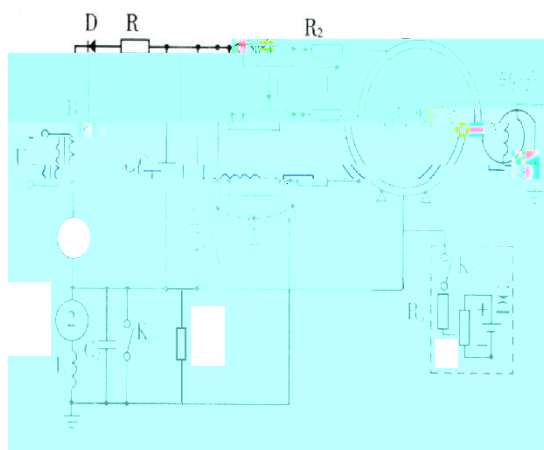

4.1

4-1

4-2

A.

4-1

1.

320X240

LCD

4-3

4-7
2.
3.

“ ”
4.
5.

6.

7. /

“ ”

“ ”

8.

9.

10. 1A

11.

12.





11

13. AC 380V ± 10% 50/60Hz

4mm2

C.

4-3 4-7

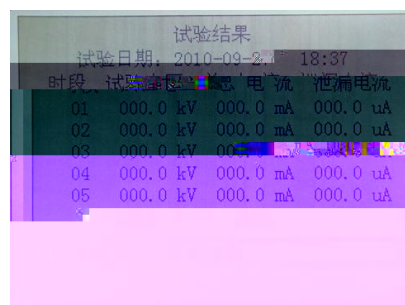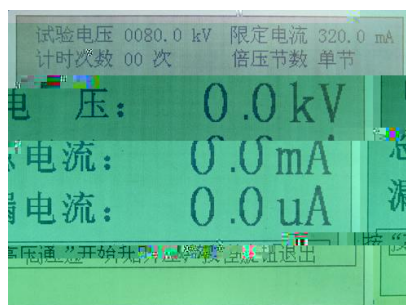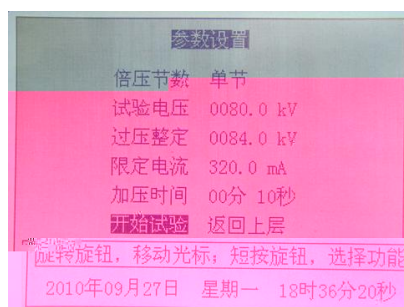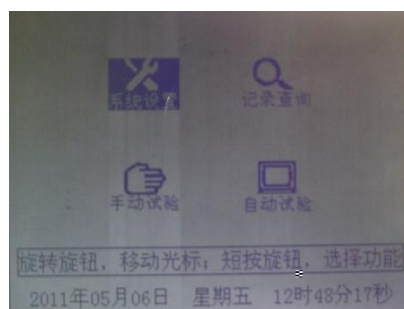

试验结果			
试验日期: 2010-09-26 19:40			
时段	试验电压	总 电 流	泄漏电流
01	012.4 kV	041.3 mA	000.3 uA
02	022.1 kV	074.7 mA	001.1 uA
03	034.0 kV	115.8 mA	009.6 uA
04	046.7 kV	160.5 mA	033.7 uA
05	055.2 kV	180.2 mA	050.1 uA
打印 上一页 下一页 返回			
旋转旋钮, 移动光标; 短按旋钮, 选择功能			
共02页 第02页			

4.1.1

4-3 /

4.1.2

4-4

“ ”

1.1

4.1.3

4-5

1-1 mA 1

100Ω

1-1 μA 1

10kΩ

3mA

4.1.4

4-6


1/3

15

4.1.5

4-7

4.2

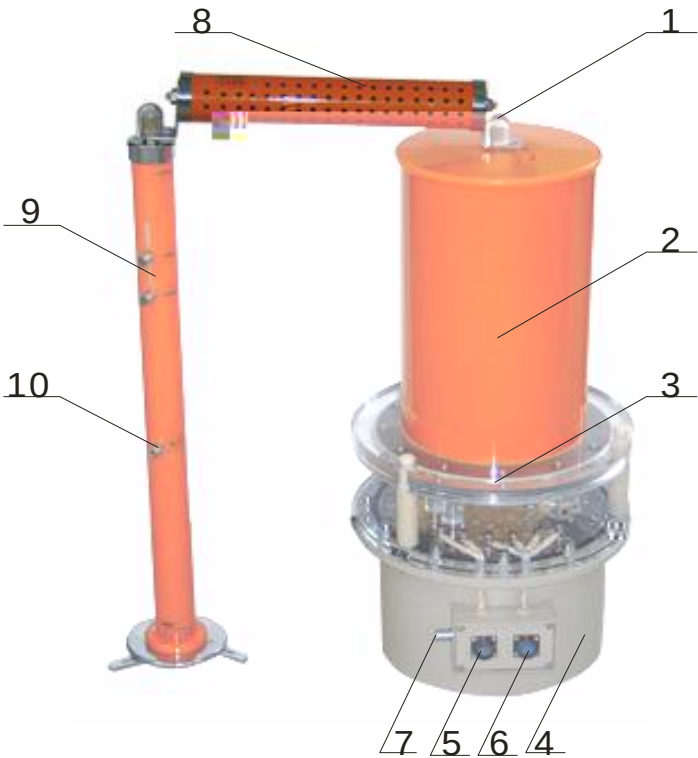

1		2
3		4
5		6
7		8
9	(	1mA 30kV 40kV 50kV 60kV)
10	(	" ")
	5	/

[REDACTED]

5.1

[REDACTED]

5.1.1

5.1.2

6

ZGS

6

$\leq 1\text{mA}$

5.2

5.2.1

,

5.2.4

5.2.5

5.2.6

mA

μA

mA

$\leq 1\text{mA}$

mA

mA


5.2.7

5.3

5.3.1f

5.1-5.2

. J, t

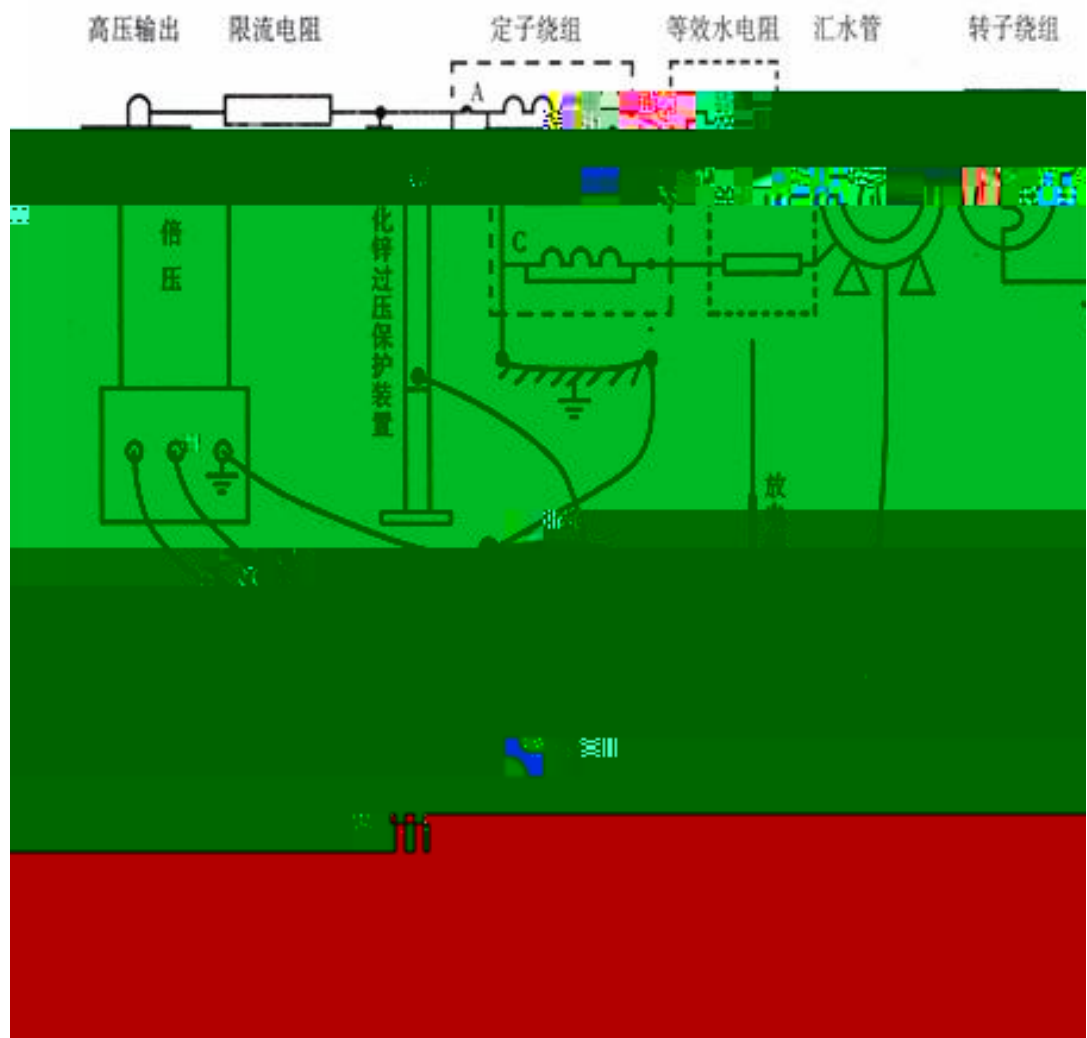

5.4

5.4.1

27.6kV 30kV
30kV

40kV 50kV

5.4.2

10KΩ

10KΩ

1KΩ

5.4.3

5.4.3.1

5.4.3.2

5.4.3.4

5.4.3.5

